

Cephalometric measurements from 3D reconstructed images compared with conventional 2D images

Natalia Zamora^a; Jose M. Llamas^b; Rosa Cibrián^c; Jose L. Gandia^b; Vanessa Paredes^a

ABSTRACT

Objective: To assess whether the values of different measurements taken on three-dimensional (3D) reconstructions from cone-beam computed tomography (CBCT) are comparable with those taken on two-dimensional (2D) images from conventional lateral cephalometric radiographs (LCRs) and to examine if there are differences between the different types of CBCT software when taking those measurements.

Material and Methods: Eight patients were selected who had both an LRC and a CBCT. The 3D reconstructions of each patient in the CBCT were evaluated using two different software packages, NemoCeph 3D and InVivo5. An observer took 10 angular and 3 linear measurements on each of the three types of record on two different occasions.

Results: Intraobserver reliability was high except for the mandibular plane and facial cone (from the LCR), the Na-Ans distance (using NemoCeph 3D), and facial cone and the Ans-Me distance (using InVivo5). No statistically significant differences were found for the angular and linear measurements between the LCRs and the CBCTs for any measurement, and the correlation levels were high for all measurements.

Conclusion: No statistically significant differences were found between the angular and linear measurements taken with the LCR and those taken with the CBCT. Neither were there any statistically significant differences between the angular or linear measurements using the two CBCT software packages. (*Angle Orthod.* 2011;81:856–864.)

KEY WORDS: 2D; 3D; CBCT; LCR; Cephalometric; Measurement

INTRODUCTION

Cephalometric analysis is one of the key tools in undertaking an accurate diagnosis in orthodontics, even though it presents a number of limitations given that it reduces to two dimensions a three-dimensional (3D) object by projecting all structures onto a single plate, thereby creating difficulties when it comes to understanding and undertaking an adequate analysis. More-

over, cephalometric analysis has other technical limitations as the images obtained can be distorted because of mistakes associated with the X-ray apparatus or errors in the positioning of the patient's head.

Conventional medical computed tomography (CT) was developed to analyze 3D structures on the three spatial planes and so provide a more realistic image, although the high cost of 3D reconstruction and the high dosage of radiation involved limited its use. Cone-beam computed tomography (CBCT)^{1,2} was then developed to reduce the radiation dosage, achieve greater precision on the three spatial planes, and reduce the costs associated with CT.³

The accuracy^{4–16} and reproducibility^{11,14} of cephalometric landmarks have been widely studied for CT^{4,17,18} and CBCT^{5,10,12,13,19} by evaluating the location of those landmarks²⁰ or by comparing the linear and angular measurements^{15,21–23} taken on lateral cephalometric radiographs (LCR) with two-dimensional (2D) projections (orthogonal, in perspective, maximum-intensity projection [MIP], projection similar to x-ray [RaySum]), obtained from slices of a CBCT scan. The results for landmark location were similar for both methods,^{20–22}

^a Assistant Professor, Department of Orthodontics, Faculty of Medicine and Dentistry, University of Valencia, Valencia, Spain.

^b Professor and Director of Postgraduate Orthodontics Masters Course, Department of Orthodontics, Faculty of Medicine and Dentistry, University of Valencia, Valencia, Spain.

^c Associate Professor, Department of Physiology, Faculty of Medicine and Dentistry, University of Seville, Seville, Spain.

Corresponding author: Dra Natalia Zamora Martínez, Clínica Odontológica, Departamento Ortodoncia 5º piso, c/ Gasco Oliag nº1, 46010 Valencia, Spain (e-mail: nataz84@hotmail.com)

Accepted: February 2011. Submitted: December 2010.

Published Online: April 7, 2011

© 2011 by The EH Angle Education and Research Foundation, Inc.

Table 1a. Definition of the Three Spatial Planes of the 17 Cephalometric Landmarks Used in This Study

Name	Anatomical Definition	Sagittal or Lateral View	Coronal or Frontal View	Axial View
Sella turcica (S)	Anteroposterior midpoint of the pituitary fossa of the sphenoid bone	Midpoint of the anteroposterior width	Midpoint of the lateral width of the fossa, determined anteroposteriorly by the other two slices	Midpoint of the anteroposterior and lateral width of the fossa
Nasion (Na)	Most anterior point of the frontonasal suture	Most anterior point	Midpoint	Most anterior and midpoint of the anterior contour
Basion (Ba)	Most anterior point of the foramen magnum	Most posterior and lowest point	Midpoint of the foramen, determined anteroposteriorly by the other two slices	Most anterior point of the foramen
Right porion (Por)	Uppermost and midpoint of the external right roof of the auditory meatus	Uppermost and midpoint	Uppermost point	Midpoint, determined superoinferiorly by the other two slices
Pogonion (Pg)	Most anterior point of the mandibular symphysis	Most anterior point	Midpoint	Most anterior and midpoint
Gnathion (Gn)	Most anteroinferior point of the mandibular symphysis	Most anterior and lowest point	Mid- and lowest point	Most anterior, lowest and midpoint
Menton (Me)	Lowest point of the mandibular symphysis	Lowest point	Lowest point	Lowest and midpoint
Anterior nasal spine (Ans)	Most anterior point of the maxillary process in the nasal floor region	Most anterior point	Most anterior and midpoint	Most anterior and midpoint
Posterior nasal spine (Pns)	Most posterior and midpoint of the palatine bone contour	Most posterior point	Most posterior and midpoint	Most posterior and midpoint
Right gonion (Gor)	Most posterior point of the posterior edge of the right branch. Bisection of the tangents of the posterior edge of the branch and the lower body	Most posterior point	Most posterior and midpoint	Most posterior point, determined superoinferiorly by the other two slices
Right orbital (Orr)	Most anterosuperior point of the infraorbital margin of the right orbital	Most anterior point	Uppermost and midpoint	Most anterior point
Incisal edge of upper right central incisor (UIr)	Lowest point of the incisal edge of the UIr	Lowest point	Most mesial point of the mesiodistal width	Most anterior and mesial point
Apical root of upper right central incisor (UIrroot)	Uppest point of the apical root of the UIrroot	Uppest point	Most uppest of the mesiodistal width	Most central point
Incisal edge of lower right central incisor (LIr)	Uppest point of the incisal edge of the LIr	Uppest point	Most mesial point of the mesiodistal width	Most anterior and mesial point
Apical root of lower right central incisor (LIrroot)	Lowest point of the root of the LIrroot	Lowest point	Most lowest point of the mesiodistal width	Most central point
Point A (A)	Most posterior point of the maxillar curvature, between the anterior nasal spine and the supradental point	Most posterior point	Midpoint determined anteroposteriorly by the other two slices	Most anterior and midpoint
Point B (B)	Most posterior point of the anterior surface of the mandibular symphysis	Most posterior point	Midpoint determined anteroposteriorly by the other two slices	Most anterior and midpoint

greater reproducibility being found in the projections from CBCT than from LCR, although there were no clinically significant results.²³ It has also been observed that the RaySum projection is more reproducible than the MIP and that either projection could replace LCR, thus making LCRs unnecessary when a CBCT has previously been undertaken on a patient.^{15,21–23}

However, for frontal projections, other authors found statistically significant differences, as they saw that the

positioning of the patient's head²⁴ influenced the measurement.

Other studies concluded that in order to adjust the location of cephalometric landmarks, slices were more accurate than the 3D view provided, because 3D projection did not represent real surfaces.¹⁴ Nevertheless, these results differed from those of other studies that found linear measurements undertaken directly on 3D images to be more accurate.²⁵

Table 1b. Description of Angular and Linear Measurements Used in This Study

Angular measurements	SNA	Angle between point S, point Na, and point A
	SNB	Angle between point S, point Na, and point B
	NS-Palatal plane	Angle between Na-S line and Ans-Pns line
	NS-Mandibular plane	Angle between Na-S line and Gor-Gn line
	Interincisal angle	Angle between Ulrroot-Ulr line and Lir-Llrroot line
	Upper incisor-NS	Angle between Na-S line and Ulrroot-Ulr line
	Tweed angle	Angle between Gor-Gn line and Lir-Llrroot line
	Facial cone	Angle between Na-Pg line and Gor-Gn line
	Cranial deflexion	Angle between Na-Ba line and Orr-Por line
	Facial depth	Angle between Na-Pg line and Orr-Por line
Linear measurements	Na-Me	Length between point Na and point Me
	Na-Ans	Length between point Na and point Ans
	Ans-Me	Length between point Ena and point Me


As there are few studies that compare the cephalometric values obtained from LCR with those from 3D projection of CBCT, and as we wanted to determine the compatibility of different CBCTs in common cephalometric analyses, the aims of our study were, first, to check whether the angular and linear measurements of 3D reconstructions obtained from a CBCT are equal to those of 2D images obtained from the LCR, and second, to check whether there are differences between two CBCT software packages (Beta Nemoceph 3D, Software Nemotec, SL, Madrid,

Spain and InVivo5 Anatomage, San Jose, Ca) when taking those measurements.

MATERIALS AND METHODS

The sample was distributed as follows: four women and four men between the ages of 8 and 30 years old. Mean ($\pm$ SD) age = 15.55 ± 6.25 years old.

Eight patients were selected. Those patients had undergone both an LCR and a CBCT before treatment and within 3 months of each other. The CBCTs had

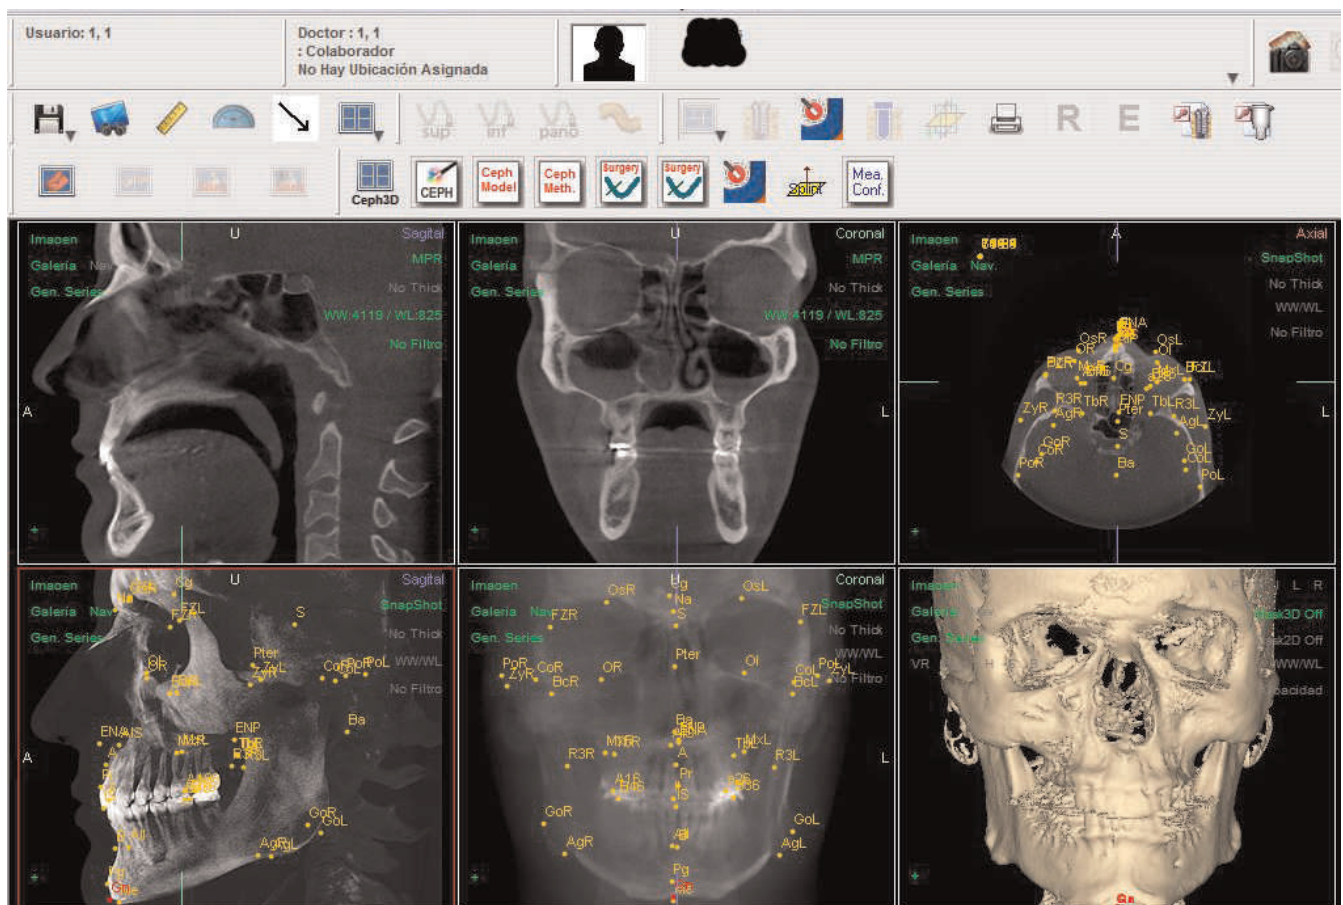**Figure 1.** Location of the cephalometric landmarks in the Beta NemoCeph 3D® software package.

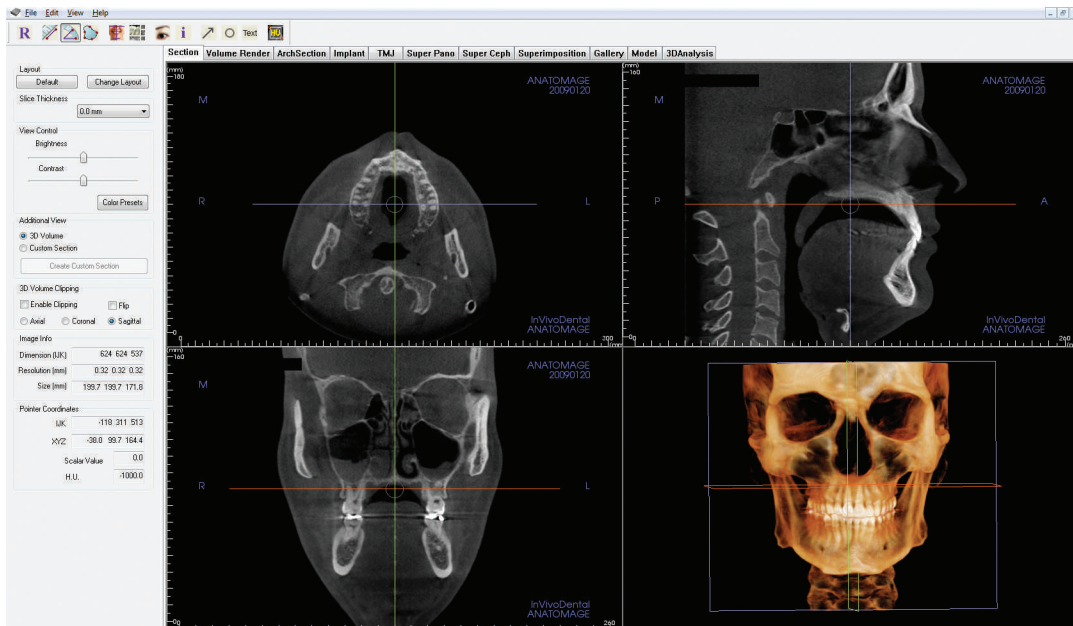


Figure 2. Location of the cephalometric landmarks in the InVivo5® software package.

been taken because some of these patients were going to undergo orthognathic surgery and the others presented with inclusions of maxillary canines.

The LCRs were taken using a cephalostat Orthophos Plus DS (Sirona Dental Systems GmbH, Germany) with a radiation time of 16 seconds for an exposure time of 0.4 seconds, the tube voltage being 73 kV and the intensity 15 mAs, whereas the CBCTs were taken using i-CAT equipment (Imaging Sciences International, Hatfield, Pa) that generates a total of 326 slices, with an image matrix size of 400 × 400 in medium-quality and high-resolution mode. The field of view (FOV) used was the portrait mode, which gathers data in extended

FOV mode and covers the full skull of 170 mm in height × 230 mm in diameter with a scanning time of 8.9 seconds. Voxel size was 0.4 × 0.4 × 0.4 mm, the tube voltage being 120 kV and the intensity 23.87 mAs. The size of the data files created is 35 megabytes.

To carry out this study, 17 cephalometric landmarks were located. These are described from the three spatial planes in Table 1a. Then, 10 angular and 3 linear measurements were taken (Table 1b).

The LCRs were digitalized using a conventional scanner-type HP Scan Jet II Cx/T (Hewlett Packard Development Company LP, Palo Alto, Ca), and the location of the landmarks was measured using the

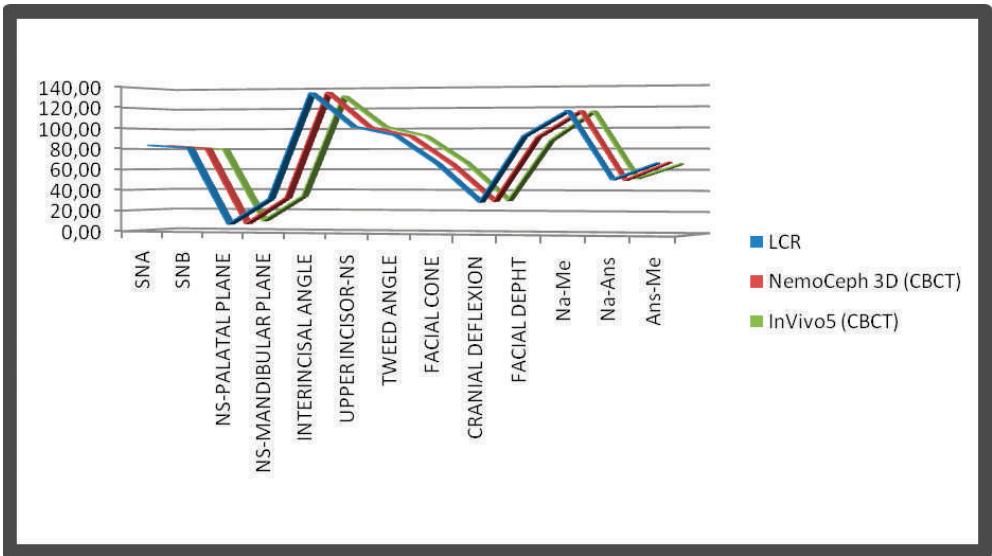


Figure 3. Comparison between the three methods. Means of all values provided.

Table 2. Intraobserver Reliability Between the First and Second Measurement*

Measurement	LCR			CBCT (NemoCeph 3D)		
	Mean ± SD	1st–2nd Measurement	P value of the Mean	Mean ± SD	1st–2nd Measurement	P value of the Mean
SNA	83.36 ± 5.24	0.990	.782	83.08 ± 4.22	0.932	.314
SNB	80.68 ± 6.91	0.994	.697	80.29 ± 6.07	0.979	.450
NS-Palatal plane	7.53 ± 6.25	0.939	.822	7.02 ± 6.20	0.976	.198
NS-Mandibular plane	31.98 ± 6.62	0.983	.013*	32.57 ± 6.35	0.951	.322
Interincisal angle	133.10 ± 9.24	0.940	.479	134.51 ± 1.34	0.987	.637
Upper Incisor-NS	100.80 ± 8.27	0.915	.497	100.8 ± 8.95	0.969	.184
Tweed angle	92.51 ± 8.93	0.953	.281	91.92 ± 8.02	0.953	.703
Facial cone	65.43 ± 6.34	0.983	.022*	64.81 ± 5.69	0.979	.190
Cranial deflexion	29.84 ± 2.35	0.509	.547	30 ± 2.30	0.985	.783
Facial depth	91.36 ± 5.15	0.872	.542	90.73 ± 5.32	0.976	.586
Na-Me	114.70 ± 8.16	0.989	.598	115.21 ± 0.56	0.997	.263
Na-Ans	51.18 ± 3.13	0.802	.519	50.36 ± 3.69	0.972	.003*
Ans-Me	66.36 ± 6.79	0.915	.679	67.08 ± 6.70	0.997	.340

* Statistically significant difference at $P \leq .05$.

Nemotec Dental Studio NX program (Software Nemotec SL, Madrid, Spain).

The raw data and slices obtained from the CBCTs were imported to two different software packages where 3D reconstruction was undertaken. Location of the cephalometric landmarks for each of the two CBCT software packages was undertaken by creating different types of projections (multiplanar reconstruction, RaySum, MIP) on the sagittal, coronal, and axial views and to the volumetric reconstruction (3D).

First, to fine-tune the location of points using the Beta NemoCeph 3D software (Software Nemotec SL, Madrid, Spain), two windows were created for the sagittal view and another two for the coronal or frontal view, which, moreover, can be enlarged to full screen using the zoom. By doing so, we can simultaneously observe the right and left sides or have two projections of the same side open for the sagittal view, or, for the coronal view, have two different projections open at the same time (Figure 1). To locate each landmark, the slice of the most appropriate plane was selected before fitting it onto the other planes for greater accuracy.

Second, to locate landmarks using the InVivo5 software (Anatomage, San Jose, Calif), the program allows one to view either a part or the whole skull by navigating across the slices so as to choose the most appropriate one for locating each point (Figure 2).

All measurements were undertaken by a single observer previously trained and qualified in the location of cephalometric landmarks and with six years of experience/background in orthodontics. The measurements were taken on two different occasions with an interval of one week between the first and second measurements so as to measure the intraobserver error.

All variables and measurements were introduced onto a version 12.0 Excel spreadsheet (Microsoft Corp, Redmond, Wa) and then analyzed using version

17.0 of the statistics package SPSS for Windows (IBM Corp, Somers, NY). To calculate the reproducibility of each of the systems used, a *t*-test was undertaken for related samples. To determine reliability of the different types of systems, a repeated measurement analysis of variance was undertaken using a variance factor, by means of Scheffé's adjustment for multiple comparisons, through the means obtained from the first and second observations for that purpose. Differences were considered significant at $P < .05$.

RESULTS

The results obtained from this study are shown in Tables 2 and 3 and in Figure 3.

Table 2 shows the intraobserver reproducibility between the first and second measurement for each of the methods. In the measurements taken on the LCR, a statistically significant difference can be observed in the angle of the mandibular plane, where the maximum difference between the two measurements (first and second) was determined as being 3.60° ($[3.60 \div 31.98] \times 100 = 11.25$), which means an error of 11.25%, as well as in the facial cone, with a maximum difference of 3.60° ($[3.60 \div 65.43] \times 100 = 5.5$), which means an error of 5.5%. In the measurements taken with the Beta NemoCeph 3D, a difference was found for the Na-Ans distance, with a maximum difference between measurements of 2.5 mm ($[2.5 \div 51.18] \times 100 = 5$), which means 5% of error in that measurement. Lastly, in the measurements taken with InVivo5, a statistically significant difference was found for the facial cone (maximum difference: 3.48° ; $[3.48 \div 66.15] \times 100 = 5.3$), which means 5.3% of error, and for the Ans-Me distance (maximum difference: 5.78 ; $[5.78 \div 65.46] \times 100 = 8.8$), which means an error of 8.8%.

Table 2. Extended

CBCT (InVivo5)		
Mean $\pm$ SD	1st–2nd Measurement	P value of the Mean
82.10 $\pm$ 33.90	0.881	.625
79.49 $\pm$ 5.87	0.964	.723
8.08 $\pm$ 7.31	0.990	.292
33.71 $\pm$ 5.76	0.935	.087
131.80 $\pm$ 10.51	0.899	.943
101.70 $\pm$ 8.63	0.955	.425
92.37 $\pm$ 8.85	0.863	.200
66.15 $\pm$ 6.17	0.976	.037*
30.17 $\pm$ 1.37	0.796	.076
89.02 $\pm$ 4.60	0.498	.115
115.70 $\pm$ 11.38	0.995	.055
51.95 $\pm$ 4.17	0.681	.695
65.46 $\pm$ 6.92	0.960	.028*

Table 3 shows the correlations between the three types of methods, and the correlations between the three methods are high. Only the facial cone (between LCR and InVivo5) presented lower values.

DISCUSSION

Each of the 13 variables used in this study were measured on the LCR and on the 3D reconstruction of each CBCT using the two software packages (Beta NemoCeph 3D and InVivo5) in order to compare their reproducibility and the statistically significant differences between each of the methods for the measurements analyzed.

To determine the reproducibility of the measurements and the intraobserver error, a single observer repeated all the measurements on a second occasion. We consider that it is sufficient to do so twice, as additional measurements do not provide any relevant additional information.²⁶ Moreover, the possible systematic errors made by an observer will always be the same for the three methods. If the measurements of more observers are combined, they may lead to errors when it comes to evaluating the real variability of the measurements.²⁶

In general, reproducibility between the first and the second measurement, both for the linear and angular measurements, was high for all three methods, with correlation indices of intraclass correlation > 0.86 in all cases except for cranial deflection and the Na-Ans distance on the LCR and InVivo5 and for facial depth with the InVivo5 software package.

The only statistically significant differences found were between the first and second measurement for the SNa-mandibular plane angle and for the facial cone measured on the LCR, for the Na-Ena distance measured using the NemoCeph 3D software package,

and for the facial cone and Ans-Me distance using the InVivo5 software package.

For these measurements, a systematic error rather than a random one was found between the first and second measurements providing greater values for one measurement than the other. For this reason those measurements appear with statistically significant differences. However, in all cases the relative error determined from the maximum discrepancy has not exceeded the method error, as all the measurements taken would fall within method variability (obtained by dividing the standard deviation [SD] between the mean of each value).

On analyzing the correlations of each of the variables for the three methods, no angular or linear measurement was found with a statistically significant difference using the three techniques, although we have observed that facial depth presents the worst correlation between the three variables (between LCR and InVivo5 and between Beta NemoCeph 3D and InVivo5), which implies that there is a greater difference between the values of this measurement in the three methods.

In contrast to our results, Van Vlijmen et al.²⁷ found statistically significant differences in several measurements that were measured on the LCR and on the CBCT; for example, the SNa-mandibular plane angle and the SNB angle. However, as in our study, the difference between most of the measurements was less than the SD, confirming that that difference was not clinically significant, although reproducibility of the measurements on the LCR was higher than in the 3D reconstructions. In the cases in which a 2D line and 3D plane were used for undertaking a measurement, they observed that there may be a clinically relevant difference, so 3D tracings would not be recommendable for undertaking longitudinal studies where pre-treatment records had been recorded in 2D. However, measurements undertaken on a single patient who has 3D records would be of use for comparing pre- and posttreatment changes or changes due to growth. In another study²⁸ by the same authors, which compared 2D and 3D frontal views, clinically relevant differences were found for both types of measurement. In a third study,²⁶ the same authors compared measurements between two types of CBCT (Iluma Imtech, Ardmore, OK and iCAT, Imaging Sciences International, Inc, Hatfield, Pa), concluding that the measurement reproducibility of 3D reconstructions in Iluma was higher than in the i-CAT, finding, in addition, statistically significant differences between several angular measurements, although only two of them presented clinically relevant differences.

Yitschaky et al.²⁹ compared angular, linear, and ratio measurements between the LCR and CT and did not

Table 3. Multiple Comparisons Using the Scheffé Method

Measurement	(I)	(J)	Difference of the Mean (I-J)	Error	Significance*
SNA	LCR	NemoCeph 3D	0.27500	2.24546	.993
		InVivo5	1.22375	2.24546	.863
		NemoCeph 3D	0.94875	2.24546	.915
SNB	LCR	NemoCeph 3D	0.38125	3.14926	.993
		InVivo5	1.18000	3.14926	.932
		NemoCeph 3D	0.79875	3.14926	.968
NS-Palatal plane	LCR	NemoCeph 3D	0.51250	3.30267	.988
		InVivo5	-0.54875	3.30267	.986
		NemoCeph 3D	-1.06125	3.30267	.950
NS-Mandibular plane	LCR	NemoCeph 3D	-0.59375	3.12667	.982
		InVivo5	-1.73000	3.12667	.859
		NemoCeph 3D	-1.13625	3.12667	.936
Interincisal angle	LCR	NemoCeph 3D	-1.46250	5.19933	.961
		InVivo5	1.27750	5.19933	.970
		NemoCeph 3D	2.74000	5.19933	.871
Uppre incisor-NS	LCR	NemoCeph 3D	0.06875	4.31088	1.000
		InVivo5	-0.90000	4.31088	.978
		NemoCeph 3D	-0.96875	4.31088	.975
Tweed angle	LCR	NemoCeph 3D	0.58750	4.30435	.991
		InVivo5	0.14125	4.30435	.999
		NemoCeph 3D	-0.44625	4.30435	.995
Facial cone	LCR	NemoCeph 3D	0.62500	3.03655	.979
		InVivo5	-0.72250	3.03655	.972
		NemoCeph 3D	-1.34750	3.03655	.907
Cranial deflexion	LCR	NemoCeph 3D	-0.16250	1.02769	.988
		InVivo5	-0.33375	1.02769	.949
		NemoCeph 3D	-0.17125	1.02769	.986
Facial depth	LCR	NemoCeph 3D	0.62500	2.51701	.970
		InVivo5	2.34125	2.51701	.654
		NemoCeph 3D	1.71625	2.51701	.795
Na-Me	LCR	NemoCeph 3D	-0.48125	5.06312	.995
		InVivo5	-0.98125	5.06312	.981
		NemoCeph 3D	-0.50000	5.06312	.995
Na-Ans	LCR	NemoCeph 3D	0.81250	1.84284	.908
		InVivo5	-0.77000	1.84284	.917
		NemoCeph 3D	-1.58250	1.84284	.696
Ans-Me	LCR	NemoCeph 3D	-0.71875	3.40104	.978
		InVivo5	0.89250	3.40104	.966
		NemoCeph 3D	1.61125	3.40104	.894

* Significance between three systems: LCR, NemoCeph 3D (CBCT), and InVivo5 (CBCT).

find statistically significant differences, except in some measurements, such as the Witts appraisal, or in others that included the Sella point (because of the differences in their location between both records). As our results, they did not find statistically significant differences for either the Na-Me or Ans-Me distances, concluding that it is possible to use most of the values previously established in 2D for measuring 3D records, as the differences between both systems were small.

Other authors have also compared angular measurements between LCR and CT.³⁰ They found only statistically significant differences in 2 of the 14 measurement that they carried out, upper incisor-Na and upper incisor-NS. However, in our study, we did not find such difference for the upper incisor-NS angle. They found, as we did, differences that were not

statistically significant for SNA, SNB, NS-palatal plane, and Tweed angle. They concluded that 3D angular cephalometric analysis was a fairly reliable method, like the traditional 2D cephalometric analysis, and that it was also more suitable for the diagnosis of cases with complex orthodontic anomalies. Currently, it could also be a suitable alternative method to 2D cephalometry with the decrease in radiation exposure and costs in the future.

To carry out this study, records of patients who had already undergone both an LCR and a CBCT for various reasons were used. Other studies have used dry skulls to undertake the measurements, as patient irradiation is not justified unless strictly necessary. However, and despite the fact that certain studies state that soft tissues distort the measurements,²⁶ it is necessary to undertake them with all the tissues

included in order to be able to check more accurately and to get as close as possible to the daily clinical reality as far as measuring patients is concerned. The drawback of carrying out a study of these characteristics is that irradiating actual patients for this purpose is not justified and therefore the sample in our study was restricted to only eight patients.

CONCLUSIONS

- No statistically significant differences were found for angular and linear measurements between the measurements taken with the LCR and those of the CBCT. The correlation indices of all measurements are very high.
- There were also no statistically significant differences for any of the angular and linear measurements between the two software packages of the CBCT (NemoStudio and InVivo5). Likewise, the correlation indices found between the different measurements were very high.

REFERENCES

1. Arai Y, Tammisalo E, Iwai K, Hashimoto K, Shinoda K. Development of a compact computed tomographic apparatus for dental use. *Dentomaxillofac Radiol.* 1999;28:245–248.
2. Mozzo P, Procacci C, Tacconi A, Martini PT, Andreis IA. A new volumetric CT machine for dental imaging based on the cone-beam technique: preliminary results. *Eur Radiol.* 1998; 8:1558–1564.
3. Mah J, Hatcher D. Diagnóstico por imagen craneofacial en ortodoncia. Capítulo 2. In: Grabber TM, Vanarsdall RL, Vig KWL, eds. *Orthodontics: Current Principles and Techniques*. St Louis, MO: Elsevier; 2005:71–100.
4. Kitaura H, Yonetsu K, Kitamori H, Kobayashi K, Nakamura T. Standardization of 3-D CT measurements for length and angles by matrix transformation in the 3-D coordinate system. *Cleft Palate Craniofac J.* 2000;37:349–356.
5. Pinsky HM, Dyda S, Pinsky RW, Misch KA, Sarment DP. Accuracy of three-dimensional measurements using cone-beam CT. *Dentomaxillofac Radiol.* 2006;35:410–416.
6. Lascala CA, Panella J, Marques MM. Analysis of the accuracy of linear measurements obtained by cone beam computed tomography (CBCT-NewTom). *Dentomaxillofac Radiol.* 2004;33:291–294.
7. Marmulla R, Wörtche R, Mühling J, Hassfeld S. Geometric accuracy of the NewTom 9000 Cone Beam CT. *Dentomaxillofac Radiol.* 2005;34:28–31.
8. Mischkowski RA, Pulsfort R, Ritter L, Neugebauer J, Brochhagen HG, Kieve E, Zöller JE. Geometric accuracy of a newly developed cone-beam device for maxillofacial imaging. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod.* 2007;104:551–559.
9. Moshiri M, Scarfe WC, Hilgers ML, Scheetz JP, Silveira AM, Farman AG. Accuracy of linear measurements from imaging plate and lateral cephalometric images derived from cone-beam computed tomography. *Am J Orthod Dentofacial Orthop.* 2007;132:550–560.
10. Moerenhout BA, Gelaude F, Swennen GR, Casselman JW, Van Der Sloten J, Mommaerts MY. Accuracy and repeatability of cone-beam computed tomography (CBCT) measurements used in the determination of facial indices in the laboratory setup. *J Craniomaxillofac Surg.* 2008;22:1–6.
11. Lagravère MO, Carey J, Toogood RW, Major PW. Three-dimensional accuracy of measurements made with software on cone-beam computed tomography images. *Am J Orthod Dentofacial Orthop.* 2008;134:112–116.
12. Stratemann SA, Huang JC, Maki K, Miller AJ, Hatcher DC. Comparison of cone beam computed tomography imaging with physical measures. *Dentomaxillofac Radiol.* 2008;37: 80–93.
13. Periago DR, Scarfe WC, Moshiri M, Scheetz JP, Silveira AM, Farman AG. Linear accuracy and reliability of cone beam CT derived 3-dimensional images constructed using an orthodontic volumetric rendering program. *Angle Orthod.* 2008;78:387–395.
14. Oliveira AE, Cevidanes LH, Phillips C, Motta A, Burke B, Tyndall D. Observer reliability of three-dimensional cephalometric landmark identification on cone-beam computerized tomography. *Oral Surg Oral Med Oral Path Oral Radiol Endod.* 2009;107:256–265.
15. Kumar V, Ludlow JB, Mol A, Cevidanes L. Comparison of conventional and cone beam CT synthesized cephalograms. *Dentomaxillofac Radiol.* 2007;36:263–269.
16. Cattaneo PM, Melsen B. The use of cone-beam computed tomography in an orthodontic department in between research and daily clinic. *World J Orthod.* 2008;9:269–282.
17. Kobayashi K, Shimod S, Nakagawa Y, Yamamoto A. Accuracy measurement of distance using limited cone-beam computerized tomography. *Int J Oral Maxillofac Implants.* 2004;19:228–231.
18. Suri S, Utreja A, Khandelwal N, Mago SK. Craniofacial computerized tomography analysis of the midface of patients with repaired complete unilateral cleft lip and palate. *Am J Orthod Dentofacial Orthop.* 2008;134:418–429.
19. Brown AA, Scarfe WC, Scheetz JP, Silveira AM, Farman AG. Linear accuracy of cone beam CT derived 3D images. *Angle Orthod.* 2009;79:150–157.
20. Grauer D, Cevidanes L, Styner MA, Heulferd I, Harmon ET, Zhuf H, Proffit WR. Accuracy and landmark error calculation using cone-beam computed tomography-generated cephalograms. *Angle Orthod.* 2010;80:286–294.
21. Cattaneo PM, Bloch CB, Calmar D, Hjortshøj M, Melsen B. Comparison between conventional and cone-beam computed tomography-generated cephalograms. *Am J Orthod Dentofacial Orthop.* 2008;134:798–802.
22. Lamichane M, Anderson NK, Rigali PH, Seldin EB, Wille LA. Accuracy of reconstructed images from cone-beam computed tomography scans. *Am J Orthod Dentofacial Orthop.* 2009;136:156.e1–6.
23. Van Vlijmen OJ, Bergé SJ, Swennen GR, Bronkhorst EM, Katsaros C, Kuijpers-Jagtman AM. Comparison of cephalometric radiographs obtained from cone-beam computed tomography scans and conventional radiographs. *J Oral Maxillofac Surg.* 2009;67:92–97.
24. Van Vlijmen OJ, Bergé SJ, Bronkhorst EM, Swennen GR, Katsaros C, Kuijpers-Jagtman AM. A comparison of frontal radiographs obtained from cone beam CT scans and conventional frontal radiographs of human skulls. *Int J Oral Maxillofac Surg.* 2009;38:773–778.
25. Hassan B, Stelt P, Sanderink G. Accuracy of three-dimensional measurements obtained from cone beam computed tomography surface-rendered images for cephalometric analysis: influence of patient scanning position. *Eur J Orthod.* 2009;31:129–134.
26. Van Vlijmen OJ, Rangel FA, Bergé SJ, Bronkhorst EM, Becking AG, Kuijpers-Jagtman AM. Measurements on 3D

- models of human skulls derived from two different cone beam CT scanners. *Clin Oral Investig*. 2010; Jul 17 (Epub ahead of print).
27. Van Vlijmen OJ, Maal T, Bergé SJ, Bronkhorst EM, Katsaros C, Kuijpers-Jagtman AM. A comparison between 2D and 3D cephalometry on CBCT scans of human skulls. *Int J Oral Maxillofac Surg*. 2010;39:156–160.
 28. Van Vlijmen OJ, Maal TJ, Bergé SJ, Bronkhorst EM, Katsaros C, Kuijpers-Jagtman AM. A comparison between two-dimensional and three-dimensional cephalometry on frontal radiographs and on cone beam computed tomography scans of human skulls. *Eur J Oral Sci*. 2009;117:300–305.
 29. Yitschaky O, Redlich M, Abed Y, Faerman M, Casap N, Hiller N. Comparison of common hard tissue cephalometric measurements between computed tomography 3D reconstruction and conventional 2D cephalometric images. *Angle Orthod*. 2011;81:13–18.
 30. Nalçacı R, Oztürk F, Sökücü O. A comparison of two-dimensional radiography and three-dimensional computed tomography in angular cephalometric measurements. *Dentomaxillofac Radiol*. 2010;39:100–106.